



# STERRAD® 100NX™

## RAISING AND EXCEEDING EXPECTATIONS.

The STERRAD® 100NX™ System is the latest advancement in low-temperature hydrogen peroxide gas plasma sterilization. It not only delivers all the reliability and performance of Next Generation (NX™) technology; it also combines increased size to meet your growing surgical demands. Truly, the premium performer in reliability and productivity.




## FEATURES

- Rectangular chamber design and four cycle options make STERRAD® 100NX™ the most productive sterilizer from ASP.
- Available as a pass-through double-door sterilizer, making it an ideal choice for installation in Central Sterilization Departments with a need for separation of clean and sterile areas.
- Large touch-screen display, foot pedal to facilitate the loading process, a diagnostic tool for troubleshooting, network connectivity for remote cycle monitoring, USB port for downloading cycle data facilitate ease of use.

Please refer to the STERRAD® 100NX™ User's Guide for more detailed processing information.

## NUMBER OF TRAYS IN 16 HOURS\*

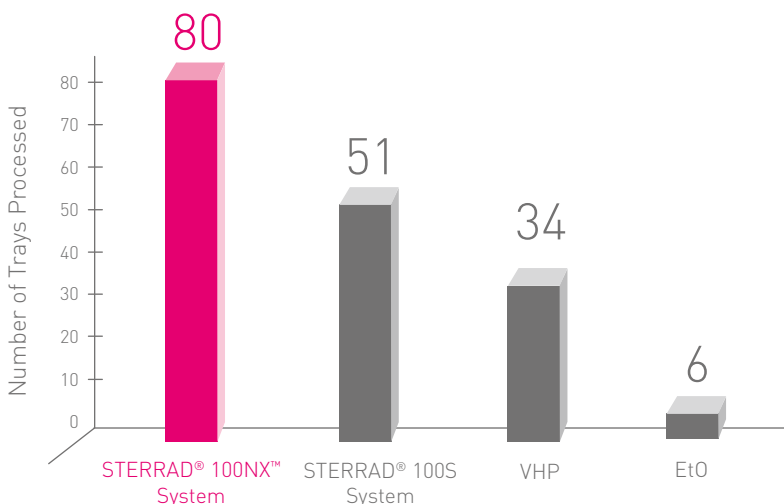

\* The number of trays processed is based on the number of 45.7 cm x 20.3 cm x 5.1 cm trays that could adequately fit in each system times the number of loads completed within 16 hours. The EtO chamber size used for this calculation is 141.6 L. The number of trays processed per load is subject to change depending on tray sizes used.

## TECHNICAL SPECIFICATIONS

TOTAL CYCLE TIME	<b>Standard Cycle</b> 47 minutes <b>Flex Cycle</b> 42 minutes <b>Express Cycle (optional)</b> 24 minutes <b>DUO Cycle (optional)</b> 60 minutes
CYCLE TEMPERATURE	Less than 55°C
DIMENSIONS & WEIGHT	<b>Height</b> 1791 mm <b>Width</b> 775 mm <b>Depth</b> 1020 mm <b>Weight</b> 425 kg single-door / 457 kg double-door
STERILIZATION CHAMBER	<b>Configuration</b> Rectangular <b>Chamber Volume</b> 152 L* <b>Dimensions</b> 410 mm x 510 mm x 735 mm <b>Two-Tiered Shelf</b> 425 mm x 700 mm
INSTALLATION & ELECTRICAL REQUIREMENTS	<b>Connections</b> 380 - 415V 50/60 Hz Power. The sterilizer requires a five-wire grounding outlet attached to a dedicated 30 AMP, 3 phase, (200-240VAC, 380-415V) ±10%, 50/60 Hz ±5% circuit with separate neutral and ground conductors.
SERVICE REQUIREMENTS	Service access requires a minimum clearance of 39.5 in (100 cm) on front, back, top and sides of the system.
OPERATIONAL ENVIRONMENT	<b>Temperature</b> 18°C to 35°C <b>Humidity</b> 10% to 85% up to 30°C, linearly decreasing from 85% at 30°C to 70% at 40°C (non-condensing)
INDEPENDENT MONITORING SYSTEM (IMS)	Enables remote, independent monitoring of all processes and is available as an option
BARCODE READER	Available as an option

\* Please contact your ASP representative to determine maximum chamber capacity based on your facility's particular sterilization load configuration(s).

## SYSTEM ORDERING INFORMATION

CODE	PRODUCT DESCRIPTION
10104	STERRAD® 100NX™ Sterilization System, single-door unit
10104-002	STERRAD® 100NX™ Sterilization System, double-door unit
10144	STERRAD® 100NX™ Cassette (2 cassettes/case; 5 cycles/cassette; 10 cycles/case)
20227	Cassette Disposal Box (10 boxes/case)
14324	STERRAD® CYCLESURE® 24 Biological Indicator (BI) (30/box; 2 boxes/case; 60/case)
10305	Thermal Printer Paper (12 rolls/case)
10142	STERRAD® 100NX™ Barcode Reader Kit
10140	Independent Monitoring System (IMS)

**FOR MORE INFORMATION** PLEASE VISIT [WWW.ASPJJ.COM/EMEA](http://WWW.ASPJJ.COM/EMEA) OR CONTACT YOUR ASP LOCAL REPRESENTATIVE

### UK:

Advanced Sterilization Products  
 A Division of J&J Medical Ltd.  
 Pinewood Campus  
 Nine Mile Ride  
 Wokingham  
 Berkshire RG40, 3EW, England  
 T: +44 1344 871 081  
 F: +44 1344 871 171

### Ireland:

Advanced Sterilization Products  
 A Division of J&J Medical Ireland  
 Airton Road, Tallaght,  
 Dublin 24, Ireland  
 T: +353 1 466 5200  
 F: +353 1 466 5340

### Egypt:

Johnson & Johnson Medical Egypt  
 Florida Mall  
 5th Floor  
 1229 Square El Sheikh Ali Gad El  
 Hak St. Heliopolis  
 Cairo, Egypt  
 T: +202 2268 5026  
 F: +202 2268 4674

### Middle East:

Advanced Sterilization Products  
 A Division of J&J Medical Middle East  
 Dubai Healthcare City, J&J building,  
 3rd floor  
 PO Box 505080, Dubai,  
 United Arab Emirates  
 T: +971 4 429 7235  
 F: +971 4 429 7250

### South Africa:

Advanced Sterilization Products  
 A Division of J&J Medical Pty.  
 Ltd. SA  
 PO Box 273, Midrand  
 Halfway House  
 1685  
 South Africa  
 T: +27 11 265 1120  
 F: +27 11 265 1189

## ADVANCED STERILIZATION PRODUCTS

Division of Medos International Sàrl

a **Johnson & Johnson** company

# SPEED AND FLEXIBILITY IN A COMPACT SIZE

With the STERRAD® NX™ System, terminally sterilized instruments are readily available to help you keep your OR ahead of schedule while providing the highest level of sterility assurance for your patients.

## RAPID TURNAROUND

- You can process up to two full rigid sets in 28 minutes or one single-channel flexible endoscope in 38 minutes
- Terminally sterilized devices maintain sterility so they can be used immediately or be stored for later use


## FLEXIBILITY

- Small enough for placement in almost any area including OR substerile rooms, OR surgical cores and specialty departments where rapid instrument turnaround is critical
- Gentle low-temperature, moisture-free environment allows you to potentially decrease damage and lower repair costs on your most delicate instruments

## PROCESSING CAPABILITY

- Offers unsurpassed monitoring including the STERRAD® CYCLESURE® 24 Biological Indicator (BI) for evidence of proper sterilization
- Delivers a Sterility Assurance Level (SAL) of  $10^{-6}$ , the highest standard of care for patients
- The STERRAD® Systems brand has the most MDM IFU endorsements for low-temperature sterilization

## OVER 100% MORE TRAYS PROCESSED\*

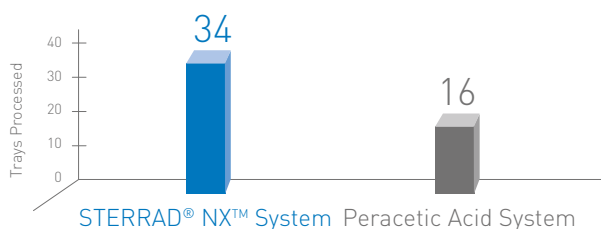


\* The number of trays processed is based on 28-minute cycle for STERRAD® NX™ System for general surgical instruments. Calculation factored 45.7 cm x 20.3 cm x 5.1 cm trays times the number of loads completed in 8 hours in STERRAD® NX™ System. Peracetic acid tray compared was the directed-flow processing container/tray, with cycle time factored at 30 minutes. Final calculation is based on the number of directed-flow processing containers/trays times the number of loads completed in 8 hours in peracetic acid system.



## TECHNICAL SPECIFICATIONS

TOTAL CYCLE TIME	<b>STANDARD Cycle</b>	28 minutes	
	<b>ADVANCED Cycle</b>	38 minutes	
CYCLE TEMPERATURE	Less than 55°C		
DIMENSIONS		SYSTEM ONLY	SYSTEM WITH CART
	<b>Height</b>	83.4 cm	157.7 cm
	<b>Width</b>	55.9 cm	60.9 cm
	<b>Depth</b>	80.6 cm	88.8 cm
	<b>Chamber Shape</b>	Rectangular	
	<b>Two-Tiered Shelf</b>	(WxD) 31.2 cm x 59.9 cm	
INSTALLATION & ELECTRICAL REQUIREMENTS	<b>Placement</b>	ASP recommends mounting your system on the specially designed cart that can be ordered with the STERRAD® NX™ System or on a countertop that meets specifications.	
	<b>Connections</b>	Single phase dedicated circuit with dedicated hot and neutral wires. Wire gauge sufficient to maintain 220–240 VAC w/ 10 amp continuous & 20 amp momentary current.*	
OPERATIONAL ENVIRONMENT	<b>Temperature</b>	18°C to 35°C	
	<b>Humidity</b>	Humidity 10% to 85% up to 30°C ambient, linearly decreasing from 85% at 30°C to 70% at 35°C	

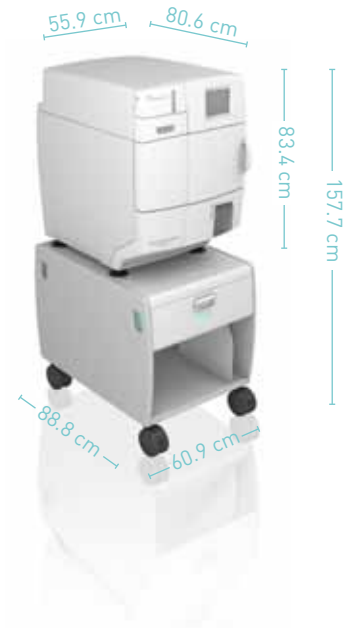

## SYSTEM ORDERING INFORMATION

All STERRAD® NX™ Systems include base unit, validation kit, installation and one-year warranty.

CODE	PRODUCT DESCRIPTION
10033	STERRAD® NX™ Sterilization System
10300	STERRAD® NX™ System Cart with locking wheels
10133	STERRAD® NX™ System Cassette (5 cycles/cassette; 5 cassettes/case)
14324	STERRAD® CYCLESURE® 24 Biological Indicator (BI) (30/box; 2 boxes/case; 60/case)†
10305	Thermal Printer Paper (12 rolls/case)
10306	Cassette Collection Box (10 boxes/case)
10308	STERRAD® NX™ System Barcode Reader
61-52645-001	Stylus
99920	STERRAD® NX™ System User's Guide

\*The STERRAD® NX™ Sterilizer has a vacuum pump which will cause the sterilizer to draw up to 20 amps of current for 1 to 2 seconds when the pump starts. If the wire gauge is too small, when the vacuum pump starts the line voltage at the outlet will drop to a level which can cause the sterilizer to reboot. Have the electrician use a voltage drop calculator to ensure the line voltage at the outlet does not drop below 198 Volts AC during the 1 to 2 seconds of 20 amps current draw.

**FOR MORE INFORMATION PLEASE VISIT [WWW.ASPJJ.COM/EMEA](http://WWW.ASPJJ.COM/EMEA) OR CONTACT YOUR ASP LOCAL REPRESENTATIVE**

### UK:

Advanced Sterilization Products  
A Division of J&J Medical Ltd.  
Pinewood Campus  
Nine Mile Ride  
Wokingham  
Berkshire RG40, 3EW, England

T: +44 1344 871 081  
F: +44 1344 871 171

### Ireland:

Advanced Sterilization Products  
A Division of J&J Medical Ireland  
Airton Road, Tallaght,  
Dublin 24, Ireland

T: +353 1 466 5200  
F: +353 1 466 5340

### Egypt:

Johnson & Johnson Medical Egypt  
Florida Mall  
5th Floor  
1229 Square El Sheikh Ali Gad El  
Hak St. Heliopolis  
Cairo, Egypt

T: +202 2268 5026  
F: +202 2268 4674

### Middle East:

Advanced Sterilization Products  
A Division of J&J Medical Middle East  
Dubai Healthcare City, J&J building,  
3rd floor  
PO Box 505080, Dubai,  
United Arab Emirates

T: +971 4 429 7235  
F: +971 4 429 7250

### South Africa:

Advanced Sterilization Products  
A Division of J&J Medical Pty.  
Ltd. SA  
PO Box 273, Midrand  
Halfway House  
1685  
South Africa

T: +27 11 265 1120  
F: +27 11 265 1189

## ADVANCED STERILIZATION PRODUCTS

Division of Medos International Sàrl

a **Johnson & Johnson** company

# PROVEN PERFORMANCE FOR COST-EFFECTIVE STERILIZATION

Using our original, innovative gas plasma technology, the STERRAD<sup>®</sup> 100S System has been a pioneer in low-temperature sterilization for nearly twenty years. Recognized for its proven performance, the STERRAD<sup>®</sup> 100S System is your cost-effective choice for dry, low-temperature sterilization.



## SAFETY

- Low temperature gas plasma efficiently eliminates traces of residual hydrogen peroxide from materials and devices and the process by-products are non-toxic oxygen and water vapor.

## SIMPLICITY

- Ease of use: one-button operation
- No costly plumbing, ventilation, or monitoring required

## COMPATIBILITY


- Proven claims\* for a wide range of material and lumens
- Capable of sterilizing rigid and flexible endoscopes, cameras, light cables, batteries, lenses, probes, microsurgical and general surgery instruments

ADVANCED STERILIZATION PRODUCTS

Division of Medos International Sàrl  
a **Johnson & Johnson** company


## HYDROGEN PEROXIDE GAS PLASMA TECHNOLOGY

Vaporized Hydrogen Peroxide (H<sub>2</sub>O<sub>2</sub>) is introduced into a vacuum chamber

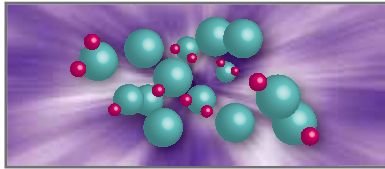

**Sterility Assurance Level: 10<sup>-6</sup>**

Plasma is generated to safely eliminate residual H<sub>2</sub>O<sub>2</sub>

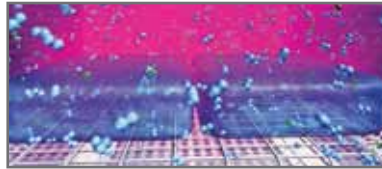

**SAFE FOR INSTRUMENTS**

System byproducts are oxygen and water



**SAFE FOR ENVIRONMENT**

## TECHNICAL SPECIFICATIONS

TOTAL CYCLE TIME	Short Cycle: 54 minutes Long Cycle: 72 minutes	
CYCLE TEMPERATURE	Less than 55°C	
DIMENSIONS & WEIGHT	<b>Height</b>	1664 mm
	<b>Width</b>	762 mm
	<b>Depth</b>	1046 mm
	<b>Weight</b>	350 kg
STERILIZATION CHAMBER	<b>Configuration</b>	Circular
	<b>Chamber Volume</b>	173L <sup>†</sup>
	<b>Shelf Dimensions</b>	Upper shelf: 700 mm x 425 mm Lower shelf: 760 mm x 325 mm
POWER USAGE	<b>Connections</b>	380-415 VAC, 50 Hz, 10 A, 3-phase circuit with separate neutral and ground conductors. CBA phase rotation
SERVICE REQUIREMENTS	In operation, the STERRAD® 100S System should not be placed closer than 5 cm to a wall at the rear and/or sides of the system. The sterilizer should be installed in a space of sufficient size to permit access to all four sides of the system when it is rolled from the rear and/or side walls are at a distance of 3 m. Service access requires a minimum clearance of 1 m on all sides of the system.	
OPERATIONAL ENVIRONMENT	<b>Temperature</b>	10°C to 40°C
	<b>Humidity</b>	30-75% relative humidity (non-condensing)

**FOR MORE INFORMATION OR TO PLACE AN ORDER: PLEASE CONTACT YOUR LOCAL ASP REPRESENTATIVE**

**Contact for UK:**

ASP c/o J&J Medical Ltd.  
Pinewood Campus, Nine Mile Ride  
Wokingham  
Berkshire RG40 3EW, England  
T : +44 1 344 871 081  
F : +44 1 344 871 171

**Contact for Ireland:**

ASP c/o J&J Medical Ireland  
Airton Rd, Tallaght  
Dublin 24, Ireland  
T : +353 1 466 5200  
F : +353 1 466 5340

**Contact for Egypt:**

Johnson & Johnson Medical Egypt  
Florida Mall 5th Floor  
1229 Square El Sheikh Ali Gad  
El Hak St. Heliopolis  
Cairo, Egypt  
T : +202 2268 5026  
F : +202 2268 4674

**Contact for Middle East:**

ASP c/o J&J Medical Middle East  
Dubai Healthcare City,  
J&J building, 3<sup>rd</sup> floor  
PO Box 505080, Dubai,  
United Arab Emirates  
T : +97 1 4 429 7235  
F : +97 1 4 429 7250

**Contact for South Africa:**

ASP c/o J&J Medical Pty. Ltd. SA  
PO Box 273, Midrand  
Halfway House 1685  
Republic of South Africa  
T : +271 1 265 1120  
F : +271 1 265 1189

All rights reserved. STERRAD is a registered trademark of Advanced Sterilization Products.

\* Please refer to the STERRAD 100S Sterilization System User's Guide prior to use. Consult with the medical device manufacturer of instruments or endoscopes you intend to sterilize with any questions regarding materials compatibility.

<sup>†</sup>Please contact your ASP representative to determine maximum chamber capacity based on your facility's particular sterilization load configuration(s).

AD-100058-01-CT\_A

# ASP<sup>®</sup> STERRAD<sup>®</sup> 200

## IT SPEAKS VOLUMES.

The STERRAD<sup>®</sup> 200 System is the large-capacity, double-doored, stainless steel sterilizer that takes productivity to the next level. This fast and innovative low-temperature sterilization system is designed for high-volume healthcare facilities requiring increased efficiency and instrument throughput.




## FEATURES

- Large rectangular chamber and option of stainless steel double-door system makes this sterilizer an ideal choice for central sterilization departments, with a need for separation of clean and sterile areas.
- Two cycle options: 75 minutes for most surgical devices and 105 minutes for flexible endoscopes and instruments with longer lumens.
- Easy Installation: does not require any water source or plumbing.

Please refer to the STERRAD<sup>®</sup> 200 User's Guide for more detailed processing information.

## A HIGHER LEVEL OF PRODUCTIVITY\*

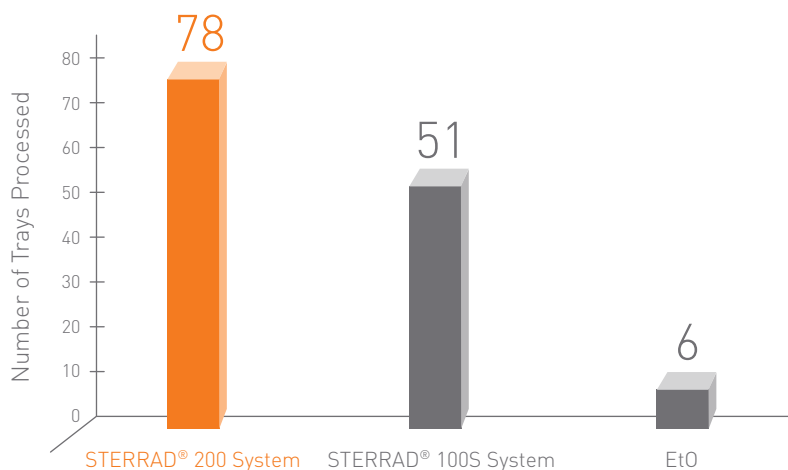

\* The number of trays processed is based on a combination of the most commonly used APTIMAX<sup>®</sup> Trays times the number of loads completed within 16 hours. The EtO chamber size used for this calculation is 141.6 L. The number of trays processed per load is subject to change depending upon tray sizes used.

## TECHNICAL SPECIFICATIONS

TOTAL CYCLE TIME	<b>Short cycle</b>	75 minutes
	<b>Long cycle</b>	105 minutes
CYCLE TEMPERATURE	Less than 55°C	
DIMENSIONS & WEIGHT	<b>Height</b>	1754 mm
	<b>Width</b>	915 mm
	<b>Depth</b>	1130 mm
	<b>Weight</b>	475 kg
STERILIZATION CHAMBER	<b>Configuration</b>	Rectangular
	<b>Chamber Volume</b>	268 L *
	<b>Two-Tiered Shelf</b>	597 mm x 597 mm (WxD)
INSTALLATION & ELECTRICAL REQUIREMENTS	<b>Placement</b>	In-wall; single-door or double-door Freestanding; single-door Built-in wheels provide mobility
	<b>Connections</b>	380-415VAC, 50 Hz, 16 A, 3-phase circuit with separate neutral and ground conductors. CBA phase rotation
SERVICE REQUIREMENTS	In operation, the STERRAD® 200 System should not be placed closer than 5 cm to a wall at the rear. The sterilizer should be installed in a space of sufficient size to permit access to all 4 sides of the system. Service access requires a minimum clearance of 1 m on all sides of the system. The power receptacle should be positioned 30.5 cm to 61 cm above the floor.	
OPERATIONAL ENVIRONMENT	<b>Temperature</b>	18°C to 40°C
	<b>Humidity</b>	10% to 85% up to 30°C ambient and linearly decreasing from 85% at 30°C to 70% at 40°C
CARRIAGE DIMENSIONS	<b>Height</b>	889 mm
	<b>Width</b>	762 mm
	<b>Depth</b>	1257 mm

## SYSTEM ORDERING INFORMATION

CODE	PRODUCT DESCRIPTION
10201-001	Single-door unit with high-density polymer resin exterior panels
10201-002	Single-door unit with stainless steel exterior panels
10202-001	Double-door unit with high-density polymer resin exterior panels
10202-002	Double-door unit with stainless steel exterior panels
10207	2-tiered shelf
10208	Carriage (4 wheels)
10118	STERRAD® 200 Cassette (5 cassettes/case; 2 cycles/cassette; 10 cycles/case)
14324	STERRAD® CYCLESURE® 24 Biological Indicator (BI) (30/box; 2 boxes/case; 60/case)
10210	Barcode reader
20226	STERRAD® 200 System Accessory Kit

\* Please contact your ASP representative to determine maximum chamber capacity based on your facility's particular sterilization load configuration(s).  
All rights reserved. STERRAD® and CYCLESURE® are registered trademarks and NXT™ is a trademark of Advanced Sterilization Products.



### UK:

Advanced Sterilization Products  
A Division of J&J Medical Ltd  
Pinewood Campus  
Nine Mile Ride  
Wokingham  
Berkshire RG40 3EW, England

T: +44 1344 871081  
F: +44 1344 871171

### Ireland:

Advanced Sterilization Products  
A Division of J&J Medical Ireland  
Airtown Road, Tallaght,  
Dublin 24, Ireland

T: +3531 466 5200  
F: +3531 466 5340

### South Africa:

Advanced Sterilization Products  
A Division of J&J Medical Pty. Ltd. SA  
PO Box 273  
Halfway House  
1685  
South Africa

T: +27 11 265 1120  
F: +27 11 265 1189

### Middle East:

Advanced Sterilization Products  
A Division of J&J Medical Middle East  
Dubai Healthcare City, J&J building,  
3rd floor  
P.O. Box 505080, Dubai,  
United Arab Emirates

T: +971 4 429 7235  
F: +971 4 429 7250

### Egypt:

Johnson & Johnson Medical Egypt  
Florida Mall  
5th Floor  
1229 Square El Sheikh Ali Gad El Hak St.  
Heliopolis  
Cairo, Egypt

T: +202 2268 5026  
F: +202 2268 4674

## ADVANCED STERILIZATION PRODUCTS

Division of Medos International Sàrl  
a Johnson & Johnson company

Advanced Sterilization Products  
a Division of Medos International Sàrl  
a Johnson & Johnson Company  
Chemin-Blanc 38, 2400 Le Locle, Switzerland



## DESIGNED FOR ALL YOUR STERILIZATION NEEDS.

Our proprietary range of complementary consumables enables your STERRAD<sup>®</sup> Systems to run reliably, safely and at maximum productivity. The sterilant used in all STERRAD<sup>®</sup> Systems is presented in a safe, easy-to-use cassette format specifically designed by Advanced Sterilization Products. Our fast-acting biological and chemical indicators, pouches, rolls and a full line of accessories were designed with your full sterilization needs in mind.



## STERILANT CASSETTES

### Our Proprietary Technology for Safe and Effective Sterilization

Our proprietary technology utilizes low-temperature hydrogen peroxide gas plasma for terminal sterilization of medical devices. Our sterilant comes in an easily loaded cassette format that delivers a predefined quantity of hydrogen peroxide per cycle to achieve sterilization both conveniently and effectively. Best of all, each cassette is a closed system, sealed for the operator's safety, and has a chemical indicator on the packaging in order to detect any leakage of sterilant during transportation. Finally, unlike some sterilization modalities, our uniquely bar-coded STERRAD® System cassettes can be transported via ground or air shipment.



## BIOLOGICAL AND CHEMICAL INDICATORS

### The Confidence of Proper Sterilization

#### BIOLOGICAL INDICATOR:

The STERRAD® CYCLESURE® 24 Biological Indicator (BI) uses *Geobacillus stearothermophilus*, tested as a highly resistant organism for hydrogen peroxide gas plasma technology, providing you with the peace of mind that proper sterilization conditions were met. In addition, the 24-hour incubation time and easy-to-read, automated process keeps your sterilization department on track.



#### CHEMICAL INDICATORS:

Designed specifically for use with your STERRAD® Sterilization System, STERRAD® SEALSURE® Chemical Indicator Tape and STERRAD® Chemical Indicator Strips use exclusive ink technology to provide an added, easy-to-read indication that the instruments have been exposed to hydrogen peroxide, leaving you confident of safe, proper processing.

## TYVEK® POUCHES AND ROLLS

### Optimal Flexibility of Chemical Indicators in a Pouch

We offer durable Tyvek® Pouches and Rolls that provide the convenience of a built-in STERRAD® Chemical Indicator, simplifying confirmation that the instruments have been exposed to hydrogen peroxide. Available in a wide variety of sizes and styles, including heat-seal and self-seal styles, our pouches and rolls reliably meet most instruments' need.



## INSTRUMENT TRAYS, MATS, AND HOLDERS

### Maximum Protection for Your Valuable Medical Devices

APTIMAX® Instrument Trays offer optimal protection for your instruments and are available in a variety of sizes to fit your instrument inventory with breakthrough, proprietary features for added protection and flexibility.



## ACCESSORIES

### Accessories to Enhance Your Convenience

A wide variety of exclusive accessories make the experience of using STERRAD® Sterilization Systems practical and efficient.



**FOR MORE INFORMATION OR TO PLACE AN ORDER: PLEASE CONTACT YOUR LOCAL ASP REPRESENTATIVE**

UK:	Ireland:	South Africa:	Middle East:	Egypt:
Advanced Sterilization Products A Division of J&J Medical Ltd Pinewood Campus Nine Mile Ride Wokingham Berkshire RG40 3EW, England T: +44 1344 871081 F: +44 1344 871171	Advanced Sterilization Products A Division of J&J Medical Ireland Airton Road, Tallaght, Dublin 24, Ireland T : +3531 466 5200 F : +3531 466 5340	Advanced Sterilization Products A Division of J&J Medical Pty. Ltd. SA PO Box 273 Halfway House 1685 South Africa T : +27 11 265 1120 F : +27 11 265 1189	Advanced Sterilization Products A Division of J&J Medical Middle East Dubai Healthcare City, J&J building , 3rd floor P.O. Box 505080, Dubai, United Arab Emirates T : +971 4 429 7235 F : +971 4 429 7250	Johnson & Johnson Medical Egypt Florida Mall 5th Floor 1229 Square El Sheikh Ali Gad El Hak St. Heliopolis Cairo, Egypt T : +202 2268 5026 F : +202 2268 4674

### ADVANCED STERILIZATION PRODUCTS

Division of Medos International Sàrl  
a Johnson & Johnson company

Advanced Sterilization Products a Division of Medos International Sàrl a Johnson & Johnson Company • Chemin-Blanc 38, 2400 Le Locle, Switzerland

All rights reserved. STERRAD®, CYCLESURE®, SEALSURE®, and APTIMAX® are registered trademarks of Advanced Sterilization Products.  
Tyvek® is a registered trademark of E.I. DuPont de Nemours and Company for its brand of protective material.

AD-090041-01-CT\_A



# ASP SteriTite® Containers: Simplicity in Instrument Packaging

ASP SteriTite® Containers provide an efficient and cost-effective way to package and protect surgical instruments for sterilization, transportation, storage, and aseptic presentation of contents.



## FEATURES AND BENEFITS

### Convenience

- Eliminates need to wrap, saving time and increasing productivity
- Easy to disassemble for cleaning and stackable for convenient storage

### Protection

- Container organizer systems protect valuable instrumentation, reducing loss and damage
- Durable construction, fully anodized and heat-treated to prevent corrosion

### Standardization

- Validated for use in STERRAD® Systems,\* steam and EtO
- Full line of reusable trays and accessories that allows you to customize instrument sets

\*Validated in the STERRAD® NX™ System, STERRAD® 100S System and STERRAD® 200 System.

# ASP SteriTite® Container Kits & Accessories



**KIT #13902**  
305 x 152 x 76 mm  
Container



**KIT #13903**  
470 x 152 x 76 mm  
Container



**KIT #13904**  
312 x 279 x 102 mm  
Container



**KIT #13905**  
460 x 279 x 102 mm  
Container



**KIT #13906**  
597 x 279 x 102 mm  
Container

CODE	DESCRIPTION: EACH KIT INCLUDES CONTAINER, INNER BASKET, INSERT BOX, NUT DRIVER, SIX 45.7 MM H POSTS, A SUPPLY OF FILTERS, LOAD CARDS AND LOCKS, AND THE FOLLOWING ADDITIONAL ACCESSORIES:
13902	8-slot brackets (one 5 mm, one 1-3 mm), single-slot brackets (two 22 mm, two 18 mm), micro stop bracket, ten hexnuts
13903	8-slot brackets (two 5 mm, two 1-3 mm), single-slot brackets (four 18 mm, two 5-10 mm, two 2-4 mm), Micro Stop Bracket, ten hexnuts
13904	15-slot 2-4 mm bracket, single-slot brackets (two 22 mm, two 18 mm, two 5-10 mm, two 5 mm, two 2-4 mm), six 68.6 mm H posts, ten hexnuts
13905	8-slot brackets (two 5 mm, two 1-3 mm), two 15-slot 2-4 mm brackets, single-slot brackets (two 18 mm, two 5-10 mm, two 5 mm, two 2-4 mm), one partition, six 68.6 mm H posts, ten hexnuts
13906	8-slot brackets (two 5 mm and two 1-3 mm), two 12-slot 5-10 mm brackets, two 15-slot 2-4mm brackets, single-slot brackets (two 22 mm, two 18 mm, two 5-10 mm, two 5 mm, two 2-4 mm, two 1-3 mm), two partitions, six 68.6 mm H posts, MediTray Micro Tray with four posts, twenty hexnuts



**FILTERS, SEALS AND LOAD CARDS**



**MEDITRAY MICRO TRAY**  
25.4 mm tray



**INSERT BOX**  
Box for Kit #13905



**INNER BASKET**  
Inner Basket for Kit #13906



**8-SLOT BACKBONE SILICONE BRACKETS**  
5 mm bracket shown



**12-SLOT BACKBONE SILICONE BRACKETS**  
5-10 mm bracket shown



**15-SLOT BACKBONE SILICONE BRACKETS**  
2-4 mm bracket shown



**SINGLE-SLOT BACKBONE SILICONE BRACKETS**  
5-10 mm & 18 mm brackets shown



**MICRO STOP BRACKET**  
139.7 L X 25.4 mm H



**PARTITION**  
238.8 L x 50.8 mm H



**POSTS**  
45.7 mm H post shown



**HEXNUT**



**NUT DRIVER**

CODE	PRODUCT DESCRIPTION	FITS CONTAINERS
13907	Round Filter (191 mm diameter)	13904, 13905, 13906
13908	Rectangular Filter (254 x 102 mm diameter)	13902, 13903
13909	Tamper-Evident Seals	Fit all containers
13910	Load Card (66 x 41 mm)	13904, 13905, 13906
13911	Load Card (25 x 44 mm)	13902, 13903

† Each accessory includes a quantity of 1,000.

**FOR MORE INFORMATION,  
PLEASE VISIT  
[WWW.ASPJJ.COM/EMEA](http://WWW.ASPJJ.COM/EMEA)  
OR CONTACT YOUR ASP LOCAL  
REPRESENTATIVE**

## ADVANCED STERILIZATION PRODUCTS

Division of Medos International Sàrl  
a **Johnson & Johnson** company



## SUPPORT YOU CAN COUNT ON.

We offer excellent service and support to ensure that your facility operates with minimum downtime and maximum predictability. We are recognized as the industry leader in service, support, and customer understanding. Our highly skilled team of field service engineers, dedicated technical support staff, and licensed clinical professionals is available to answer your questions and ensure that your facility operates efficiently and productively at all times.



## PROFESSIONAL, RESPONSIVE SERVICE AND LOGISTICS

### Field Service Engineering

ASP employs highly skilled Field Service Engineers (FSEs) who perform Planned and Corrective maintenance on STERRAD® Sterilization Systems. Our FSE team is widely seen as the most professional and responsive in the industry. Service is affordable and timely.

### Field Service Logistics

Field Service Logistics maintains a comprehensive inventory of system parts, enabling service-call completion in minimal time without sacrificing our customers' productivity.

### Installation

Our team of specialised FSEs will liaise with your hospital biomedical engineering and facilities management teams to ensure the installation of your STERRAD® conforms to national regulatory standards.

## EDUCATION AND TRAINING

### Training and Technical Centre, Strasbourg

ASP has a new purpose built facility in Strasbourg, France to host educational, technical and training meetings. Serving the EMEA region, the Strasbourg facility houses every type of STERRAD® system, so that customers can compare technologies and direct questions to our in-house European support team.

### Technical Support Training

A comprehensive range of training courses are offered from the Training and Technical Centre. Technical training courses are available throughout the year and cover ASP's range of systems; from the STERRAD® 100S to the STERRAD® 100NX™. A schedule of courses is published every January and is available on request.

### Clinical Education Consultants

ASP's Clinical Education Consultants (CECs) are registered nurses with many years of extensive industry experience. Our CECs can answer your questions about system-related issues, instrument processing, biological testing, and more. In addition, the CECs provide best practice solutions in hospitals, ambulatory, surgery centres, endoscopy centres, and clinics. Our clinicians remain on the leading edge of current hospital standards and practices to make sure they provide you with up-to-date information.

## SERVICE PROGRAMMES

ASP can provide a service programme to match your exact requirements. There may be times when one of the standard service products does not fulfil your requirements or budget. With the aim of providing maximum uptime of your department, ASP can therefore customize a service product to suit both your needs and budget.

### Warranty

All service parts, labour, and travel are covered for both planned and corrective maintenance service for one year from the date of installation, ensuring that your facility dramatically reduces downtime and keeps the sterilization process running smoothly.

### Types of Standard Service Programmes

In addition to the bespoke service products, ASP also offers standard service programmes to our customers. The standard service programmes available are:

- Parts only
- Preventative Maintenance Support
- Preventative Maintenance Support including validation
- Comprehensive Support Programme

All details of these programmes are available on request from your local office.

### ISO 14937

It is a requirement throughout EMEA to validate your STERRAD® Sterilization System to the ISO 14937 standard. ASP can provide the complete validation service for all STERRAD® systems. Our FSEs have been trained in ISO 14937 protocols and procedures and are equipped with test equipment which is traceable to national standards.

## FOR MORE INFORMATION OR TO PLACE AN ORDER: PLEASE CONTACT YOUR LOCAL ASP REPRESENTATIVE

UK:	Ireland:	South Africa:	Middle East:	Egypt:
Advanced Sterilization Products A Division of J&J Medical Ltd Pinewood Campus Nine Mile Ride Wokingham Berkshire RG40 3EW, England T: +44 1344 871081 F: +44 1344 871171	Advanced Sterilization Products A Division of J&J Medical Ireland Airtown Road, Tallaght, Dublin 24, Ireland T: +3531 466 5200 F: +3531 466 5340	Advanced Sterilization Products A Division of J&J Medical Pty. Ltd. SA PO Box 273 Halfway House 1685 South Africa T: +27 11 265 1120 F: +27 11 265 1189	Advanced Sterilization Products A Division of J&J Medical Middle East Dubai Healthcare City, J&J building , 3rd floor P.O. Box 505080, Dubai, United Arab Emirates T: +971 4 429 7235 F: +971 4 429 7250	Johnson & Johnson Medical Egypt Florida Mall 5th Floor 1229 Square El Sheikh Ali Gad El Hak St. Heliopolis Cairo, Egypt T: +202 2268 5026 F: +202 2268 4674

### ADVANCED STERILIZATION PRODUCTS

Division of Medos International Sàrl  
a Johnson & Johnson company

Advanced Sterilization Products a Division of Medos International Sàrl a Johnson & Johnson Company • Chemin-Blanc 38, 2400 Le Locle, Switzerland

All rights reserved. STERRAD® is registered trademark of Advanced Sterilization Products.