




STERRAD[®] NX[®]

DOING MORE TO MEET YOUR HYSTEROSCOPY NEEDS

Keep up with your hysteroscopy needs by optimizing your instrument flow with the STERRAD[®] NX[®] System. Our fast low-temperature hydrogen peroxide gas plasma sterilizer allows you to process typical sets of rigid scopes, cameras, bridges, sheaths, forceps and light cords required to perform a routine procedure.*

The cycle times of the STERRAD[®] NX[®] System provide you with fast turnaround for your hysteroscopy sets. The system features a 28-minute cycle time for rigid hysteroscopes and an advanced 38-minute cycle for flexible hysteroscopes. Now you can handle more caseloads with less instrument inventory, without delay. With the dry packaged, terminal sterilization process of the STERRAD[®] NX[®] System, instruments are ready for immediate use or they can be stored to use at a later time.

FAST & EASY TO USE - HYSTEROSCOPY SETS WHEN YOU NEED THEM

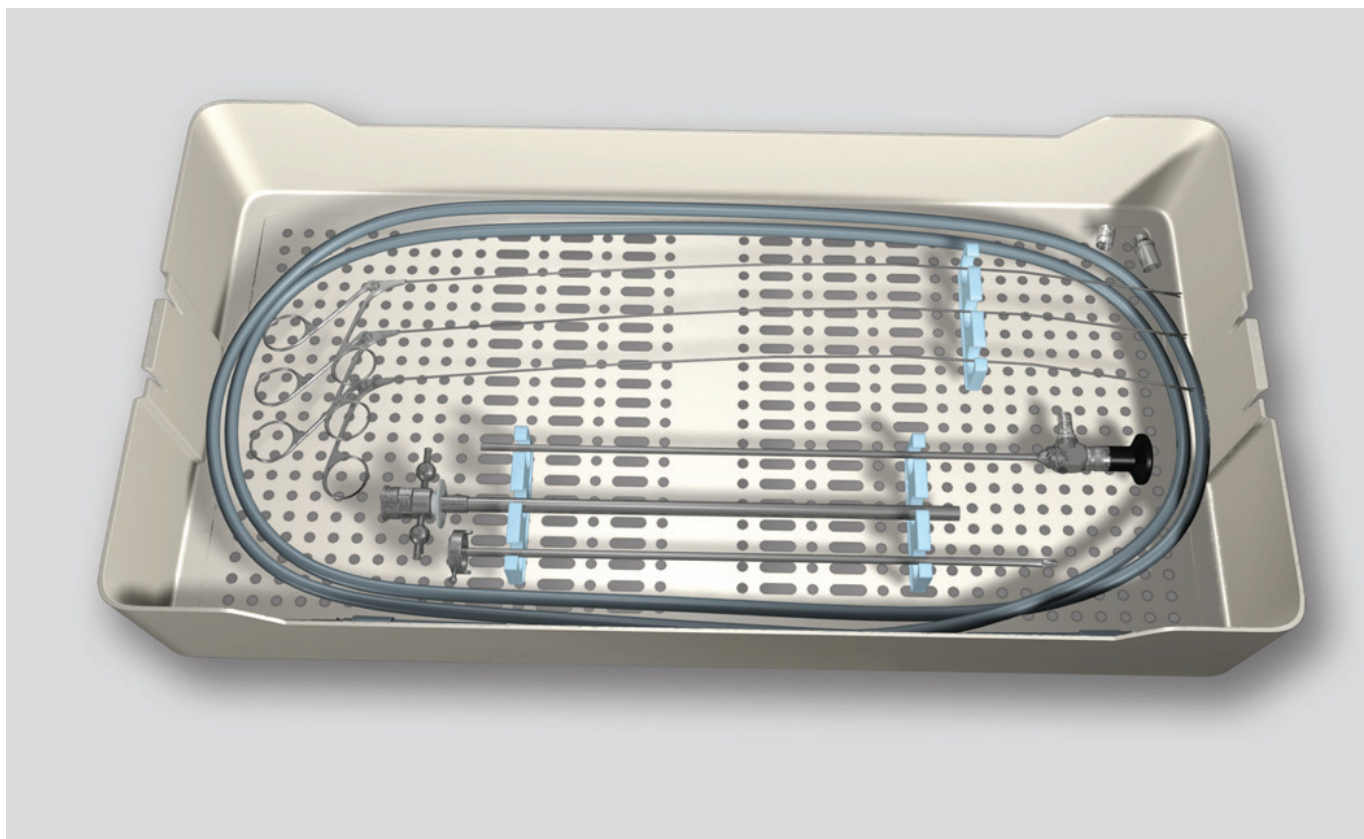

* All devices and parts must be cleaned, rinsed and dried prior to sterilization. Disassemble instruments with removable parts per the manufacturer's Instructions for Use (IFU). Remove any oil- or grease-based lubricants, as they may interfere with sterilization. After rinsing and completely drying, apply a water-based lubricant to necessary parts. For questions about whether your device can be sterilized in STERRAD[®] Systems, please refer to the manufacturer's IFU or contact the device manufacturer.



STERRAD[®] NX[®]

LET YOUR STERRAD[®] SYSTEM DO MORE FOR YOU.

TERMINALLY STERILIZED INSTRUMENTS WITHIN YOUR OR

With its compact size and easy mobility, the STERRAD[®] NX[®] System is flexible enough for placement in almost any area. This includes OR substerile rooms, OR surgical cores and specialty departments, where rapid instrument turnaround is critical. Point-of-use placement keeps your instruments close by, saves transportation time and reduces the number of instruments that can be lost or damaged in transit. With the STERRAD[®] NX[®] System close at hand, terminally sterilized instruments are readily available to keep up with your scheduling needs.



FEATURES & BENEFITS

Fast Instrument Turnaround

- 28-minute Standard Cycle for rigid hysteroscopy sets
- 38-minute Advanced Cycle for flexible hysteroscopes
- The combination of speed and the ample, two-tiered chamber helps you process up to two full rigid sets in 28 minutes or one flexible scope in 38 minutes
- Quick instrument turnaround helps ensure sets are ready when you are

Easy to Use

- Allows for sterilization of hysteroscopy sets, including cameras, in one container
- Compatible with ASP SteriTite[®] Containers and other closed container systems
- Dry, packaged, terminally sterilized instruments are ready for immediate use or can be stored for later use

Gentle On Instruments

- Provides a low-temperature and moisture-free environment that is gentler on instruments, thus potentially decreasing instrument damage and lowering repair costs

Thank you for choosing the STERRAD[®] NX[®] System. Please feel free to contact ASP at 888-783-7723, or visit www.aspjj.com if you have any questions. We look forward to helping you safely achieve sterilization in the OR.

ADVANCED STERILIZATION PRODUCTS

Division of Ethicon, Inc.

a *Johnson & Johnson* company